

# INSTRUCTIONS FOR USE

## Rickettsia Screen IFA IgG Antibody Kit

Catalog Number: R20G-120

Size: 120 test

Storage: 2-8°C

An Indirect fluorescence immunoassay for the detection and quantitative determination of IgG class antibody against both spotted fever group and typhus group Rickettsia in human serum or plasma

For in-vitro diagnostic use only



1135 E. Truslow Ave.  
Fullerton, California 92831 USA  
Phone: +1-714-525-7660  
Fax +1-714-525-7614  
Email: info@fullerlabs.com  
www.fullerlabs.com



**MediMark Europe Sarl**  
11, rue Émile Zola – BP 2332  
F-38033 Grenoble Cedex 2 – France

### INTENDED USE

The Rickettsia IFA IgG Antibody kit is intended for the simultaneous detection and semi-quantitation of IgG class human antibody to both spotted fever and typhus group Rickettsia, to be used as an aid in the diagnosis of human infection by these pathogens.

### SUMMARY AND EXPLANATION OF TEST

Spotted Fever Group Rickettsia are found worldwide and are mediated by ticks, fleas, mites and other insect vectors whose bite transfers an infection to a mammalian host. **Rickettsia rickettsii** is found throughout the western hemisphere and **Rickettsia conorii** (Boutonneuse fever) is found throughout the Mediterranean region, Africa, India and much of Asia. Many other species of spotted fever Rickettsia are also found over wide areas.

Typhus Group Rickettsia are transmitted by infected fleas and lice. This group includes **Rickettsia typhi** (endemic typhus) and **Rickettsia prowazekii** (epidemic typhus), both species found worldwide. The ensuing infections induce a specific antibody response, which may be detected and used as an indirect means of identifying an infected human.


The IFA slides in this kit utilize purified *Rickettsia rickettsii* and *Rickettsia typhi* as individual substrate antigens within each slide well. Patient sera are diluted at least 1:64 in buffered saline and incubated in the individual slide wells to allow reaction of serum antibody with the rickettsia. The slides are then washed to remove unreacted serum proteins, and an FITC-labeled anti-human IgG (Conjugate) is added, to label the antigen-antibody complexes. After further incubation, the slides are washed again to remove unreacted Conjugate. The resulting reactions can be visualized using standard fluorescence microscopy, where a positive reaction is seen as small sharply defined fluorescent rod forms within a red-counterstained background matrix. A negative reaction is seen as either counterstained (red) background or fluorescence different from that seen in the Positive Control wells. Positive reactions may then be retested at higher dilutions to determine the highest reactive or endpoint dilution.

### REAGENTS

**IFA Ag x 12**

#### Substrate Slides

10 x 12-well masked slides containing 2 acetone-fixed antigen spots in each well.

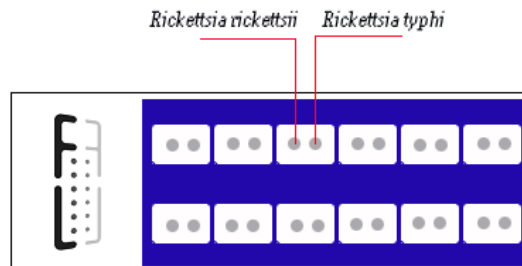

**CONJ FITC**

#### IgG Conjugate, 2.5 mL

Yellow-cap dropper bottle contains ready to use affinity-purified and DyLight 488-labeled goat anti-human IgG (heavy chain) with bovine serum albumin and Evans' blue counterstain.

**CONT +****Spotted Fever Group  
Positive Control, 0.5 mL**

Blue-cap dropper bottle contains human serum reactive against spotted fever group Rickettsia and is bottled at a 1:64 screening dilution. Endpoint titer is 1:512.

**CONT +****Typhus Fever Group  
Positive Control, 0.5 mL**

Green-cap dropper bottle contains human serum reactive against typhus group Rickettsia and is bottled at a 1:64 screening dilution. Endpoint titer is 1:512.

**CONT -****Negative Control, 0.5 mL**

Red-cap vial contains human serum non-reactive against Rickettsia and bottled at a 1:64 screening dilution.

**MM****Mounting Medium, 1 mL**

White-cap dropper bottle contains 50% glycerol in PBS.

**BUF WASH PBS****PBS, 1 liter**

Add supplied powder to 1 liter purified water to produce phosphate-buffered saline at pH 7.2.

**Warnings**

The control sera have been screened for infectious agents by USFDA required testing. Since no testing can assure the absence of infectious agents, however, these reagents, as well as all serum specimens and equipment coming in contact with these specimens, should be handled with good laboratory practices to avoid skin contact and ingestion.

The substrate slides are prepared with chemically inactivated antigens. However, the slides should be considered potentially infectious and handled accordingly.

**Storage and Handling**

Store kit components at 2-8°C or colder. Bring them to room temperature (20-25°C) before opening bottles or slide envelopes.

**SPECIMEN COLLECTION**

Allow blood samples to clot and separate sera by centrifugation. Transfer sera aseptically to tightly closing sterile containers. Store at 2-8°C. If testing is to be delayed longer than 5 days, store sera at -20°C or colder. Acute sera should be drawn at the onset of illness and convalescent sera at two and four week intervals to check for titer changes.

**PROCEDURE****Material Supplied**

The kit supplies sufficient reagents and materials for 120 determinations.

**Materials Required But Not Supplied**

- Purified (distilled or deionized) water
- Clean 250 or 500 mL wash bottle for PBS
- Wash bath with slide rack
- Test tubes or microtiter equivalent for manual dilutions
- Precision pipette(s) for making dilutions and delivering exactly 10 µL per slide well
- 24 x 50 mm glass cover slips
- Fluorescence microscope with filter system for FITC (maximum excitation wavelength 490 nm, mean emission wavelength 530 nm) and 400X magnification
- 37°C water bath or incubator
- Humidity chamber for slide incubation steps

**Precautions**

- Do not use components past expiration date.
- Conjugate is photosensitive and is packaged in opaque plastic for protection. Store in the dark and return to storage immediately after use
- Liquid components contain 0.01% thimerosal as preservative. Do not ingest.
- Conjugate contains Evans' Blue dye, which may be carcinogenic. Avoid contact with skin.

**PREPARATION OF SAMPLES AND REAGENTS**

1. **Prepare Wash Buffer** by adding contents of PBS packet to 1 liter purified water and mixing thoroughly:
2. **Prepare 1:64 dilutions** of patient sera using Wash Buffer as diluent.

**ASSAY PROCEDURE**

1. Prepare serial 2-fold dilutions in Wash Buffer of the Positive Controls to include 1 dilution above and 1 dilution below the stated endpoint (1:512). All controls are pre-diluted and bottled at 1:64
2. For each serum dilution add 10 µL to one slide well and record the location for later reference. For each assay run include the dilutions of the Positive Control prepared in step 1. Also add 1 drop of Negative Control to one well. Samples should be applied to the top or bottom edge of the well, avoiding the mid-section containing the antigen microdots.
3. Place slides into a humidity chamber and incubate for 30 minutes at 37°± 0.5°C .
4. Remove humidity chamber from incubator or water bath. Also remove conjugate from storage. Rinse slide wells with gentle stream of PBS from wash bottle three (3) times. Then allow beads of PBS to remain in the wells for at least 5 minutes.
5. Shake or tap excess PBS from slides and go directly to next step without allowing slide wells to dry.
6. To each slide well add 1 drop (10 µL) IgG Conjugate, then return slides to humidity chamber for a 30 minute incubation at 37°± 0.5°C. Incubation should be in the dark to protect the photosensitive conjugate.
7. Wash slides as in steps 5-6, above.
8. Add 2-3 drops of Mounting Medium to each slide and apply coverglass.
9. Read the stained substrate slides at 400X magnification, comparing each well to the visual intensity and appearance of the Positive and Negative Control wells. Slides may be stored at 2-8°C in the dark for up to 24 hours.

## QUALITY CONTROL

The Negative Control serum and dilutions of the Positive Controls must be assayed with each daily run. The Negative Control well is an example of a non-reactive serum, with no distinct and characteristic staining of the rickettsia. The Positive Control wells should give endpoint titers from 1:256 to 1:1024. The fluorescence intensity at 1:512 may be used as the cut-off level required for test reactions to be called positive. If any of the Controls do not react as specified, the assay run is considered void, reagent components and procedural steps should be rechecked, and the assay repeated from the beginning.

## INTERPRETATION OF RESULTS

A positive reaction appears as bright staining (at least 1+) of short pleomorphic rod forms. The size, appearance, and density of each field must be compared with the Positive and Negative Control reactions. Patterns of reactivity different from the Positive Controls must be considered non-specific.

Primary (initial) infection is characterized by a prompt rise in both IgG and IgM class antibody by IFA. IgM levels peak approximately 3 weeks post onset of symptoms and remain detectable for 2-3 months. IgG class antibody peaks in 7-12 weeks, but declines much more slowly than IgM antibody levels and remains elevated for approximately 12 months.

## PATIENT SPECIMENS

**Positive at 1:64:** IgG titers of 1:64 and greater reflect infection at an undetermined time (seropositive). Positive sera should be titered to determine their endpoint for comparison with earlier or later specimens from the same patient.

**Negative at 1:64:** Report as negative. Further sera should be drawn if the original was taken immediately post onset of symptoms, especially if antibiotic therapy was instituted.

**Positive at 1:128 and greater:** Sera giving such elevated endpoint titers suggest recent or active infection. IgM titers, when present, are also a reliable indicator of recent infection.

**Paired Sera:** A four-fold increase in titer, between acute and convalescent serum specimens, is considered strong evidence supporting the diagnosis of recent infection.

## LIMITATIONS

- In attempting to support the diagnosis of rickettsial infection in newborns the IgM class antibody should be tested for, as any IgG class antibody detected may be maternal in origin.
- A marked cross-reactivity is seen in the IFA procedure between members of the spotted fever group, which include the species *conorii*, *rickettsii*, *akari*, *parkeri*, *sibirica*, and many others. Cross-reactivity within the typhus fever group, which includes the species *typhi* and *prowazekii*, is also strong using the IFA technique.
- Cross-reactivity between spotted fever group and typhus fever group reactivity is much less evident, and titers 8-32-fold lower than those to the infecting antigenic group are observed.
- *Rickettsia felis* is a spotted fever group organism, although it is infrequently detected in this assay. Please see catalog for *R. felis*-specific assays.